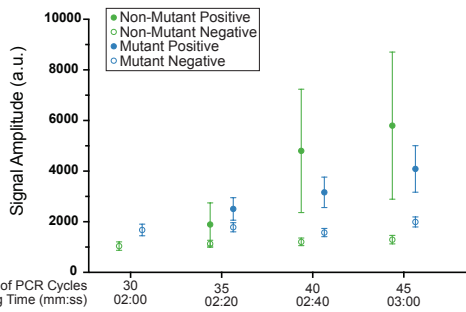
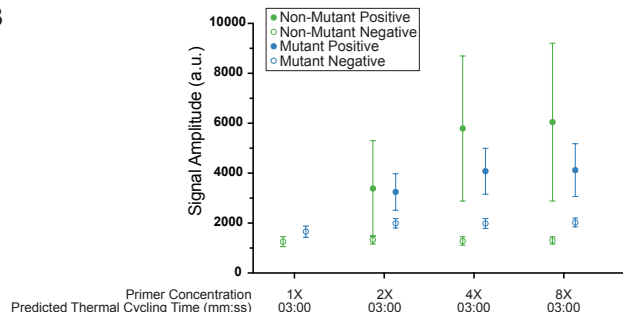


A


Constant Parameters Across Conditions:

Capillary Thermal Cycling, 1s Annealing/Extension Time, 1s Denaturation Time
 32x Aptamer HS Taq, 4x Primer, 4x Probe

B

Constant Parameters Across Conditions:

Capillary Thermal Cycling, 1s Annealing/Extension Time, 1s Denaturation Time
 45 PCR Cycles, 32x Aptamer HS Taq, 4x Probe

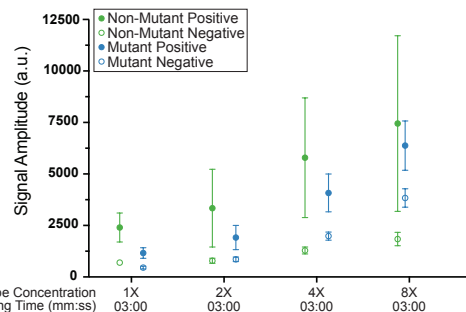C

Constant Parameters Across Conditions:

Capillary Thermal Cycling, 1s Annealing/Extension Time, 1s Denaturation Time
 45 PCR Cycles, 32x Aptamer HS Taq, 4x Primer

D