

SUPPLEMENTAL MATERIALS**Table S1. Overview of MRI scanners and sequences.**

MRI scanner	# Patients	TR (ms)	TE (ms)	Reconstructed voxel size (mm)	Slices	Inversion time (ms)	Flip angle (°)	Orientation
1. Siemens Avanto 1.5T	29	1910 - 1940	3.08 - 3.53	0.98x0.98x1; 1x1x1	144 - 176	1100	15	Sagittal
2. Siemens Sonata 1.5T	19	1980 - 3000	3.54 - 3.93	1.25x1.25x1.2; 1x1x1	120 - 160	1000	7 - 8	Sagittal
3. Siemens Avanto-fit 1.5T	9	1740	2.49	0.5x0.5x1	144 - 176	900	10	Sagittal
4. Siemens Aera 1.5T	8	1690 - 1900	2.36	0.5x0.5x1	176 - 192	900	10	Sagittal
5. Philips Ingenia 3T	6	8090 – 8360	3.69 - 3.84	0.94x0.94x1; 0.87x0.87x1	170 - 190	NA	8	Sagittal
6. Philips Ingenia 1.5T	6	7350 - 7480	3.39 - 3.43	0.5x0.5x1.1; 0.48x0.48x1.1	150 - 164	NA	8	Sagittal
7. Philips Intera 1.5T	5	8560 - 8570	3.99	0.94x0.94x1.2	132 - 145	NA	8	Sagittal
		2500	4.59 - 4.60	0.98x0.98x1.2; 0.98x0.98x1	152 - 180	NA	30	Sagittal
8. GE Medical Systems Signa HDxt 3T	3	7700 – 7770	2.94 - 2.96	1x1x1.2	166	450	12	Sagittal

Note: Different image acquisition sequences were used for the same scanner; we illustrate this variability by reporting ranges of various parameters. *Abbreviations:* Mm, Millimeters; MRI, Magnetic resonance imaging; Ms, Milliseconds; NA, Not applicable; TE, Echo time; TR, Repetition time.

Table S2. Estimates of brain morphology across MRI scanners.

MRI scanner	Mean $\pm$ SD							
	Cortical volume (mm ³)	Cortical thickness (mm)	Cortical surface area (mm ²)	Subcortical volumes (mm ³)	Cerebral WM volume (mm ³)	Cerebellar GM volume (mm ³)	Cerebellar WM volume (mm ³)	Ventricles volumes (mm ³)
1. Siemens Avanto 1.5T <i>n</i> = 29	484568.1 $\pm$ 54238.0	2.59 $\pm$ 0.10	167954.9 $\pm$ 16318.4	56925.0 $\pm$ 5248.2	451802.7 $\pm$ 58187.4	115633.8 $\pm$ 9057.0	29257.5 $\pm$ 5529.7	15312.5 $\pm$ 7870.1
2. Siemens Sonata 1.5T <i>n</i> = 19	456774.1 $\pm$ 45880.4	2.45 $\pm$ 0.12	168428.3 $\pm$ 14137.0	56543.6 $\pm$ 4507.5	469406.2 $\pm$ 44975.2	107019.9 $\pm$ 7318.0	25488.5 $\pm$ 2460.1	15807.5 $\pm$ 6970.2
3. Siemens Avanto-fit 1.5T <i>n</i> = 9	531762.2 $\pm$ 53235.4	2.56 $\pm$ 0.09	184198.9 $\pm$ 16271.6	59310.6 $\pm$ 4020.7	463354.3 $\pm$ 45345.5	123111.4 $\pm$ 9248.7	26963.5 $\pm$ 3427.6	15925.0 $\pm$ 6046.5
4. Siemens Aera 1.5T <i>n</i> = 8	482898.0 $\pm$ 34128.9	2.59 $\pm$ 0.07	165055.7 $\pm$ 12018.2	53568.3 $\pm$ 4566.5	388264.3 $\pm$ 36847.6	112964.0 $\pm$ 12418.8	27790.5 $\pm$ 6475.6	16854.9 $\pm$ 9675.3
5. Philips Ingenia 3T <i>n</i> = 6	476879.7 $\pm$ 57108.3	2.58 $\pm$ 0.11	162918.8 $\pm$ 16612.5	55466.8 $\pm$ 2977.1	404852.3 $\pm$ 42756.0	106119.7 $\pm$ 6631.0	26255.1 $\pm$ 1577.9	11446.2 $\pm$ 3193.2
6. Philips Ingenia 1.5T <i>n</i> = 6	501161.1 $\pm$ 30467.8	2.54 $\pm$ 0.10	174019.3 $\pm$ 11886.9	56316.0 $\pm$ 3930.9	402236.2 $\pm$ 24635.4	109963.3 $\pm$ 6866.8	24868.8 $\pm$ 1259.6	16523.1 $\pm$ 11415.2
7. Philips Intera 1.5T <i>n</i> = 5	503189.4 $\pm$ 22359.1	2.55 $\pm$ 0.08	175866.6 $\pm$ 6115.8	56270.2 $\pm$ 3549.0	459369.2 $\pm$ 40278.1	120179.7 $\pm$ 11543.0	28340.3 $\pm$ 2742.3	20880.3 $\pm$ 6571.2
8. GE Signa HDxt 3T <i>n</i> = 3	438574.5 $\pm$ 18744.5	2.55 $\pm$ 0.02	148584.4 $\pm$ 2519.2	50440.7 $\pm$ 2535.1	379210.1 $\pm$ 10172.9	101012.7 $\pm$ 10302.1	25782.4 $\pm$ 805.0	14617.8 $\pm$ 6365.2
All MRI scanners pooled <i>n</i> = 85	483295.8 $\pm$ 51110.3	2.55 $\pm$ 0.11	169362.1 $\pm$ 15630.0	56363.1 $\pm$ 4702.6	442050.7 $\pm$ 54707.1	112928.3 $\pm$ 10382.0	27335.7 $\pm$ 4411.9	15748.7 $\pm$ 7542.4

Abbreviations: GM, Gray matter; Mm, Millimeters; MRI, Magnetic resonance imaging; SD, Standard deviation; WM, White matter.

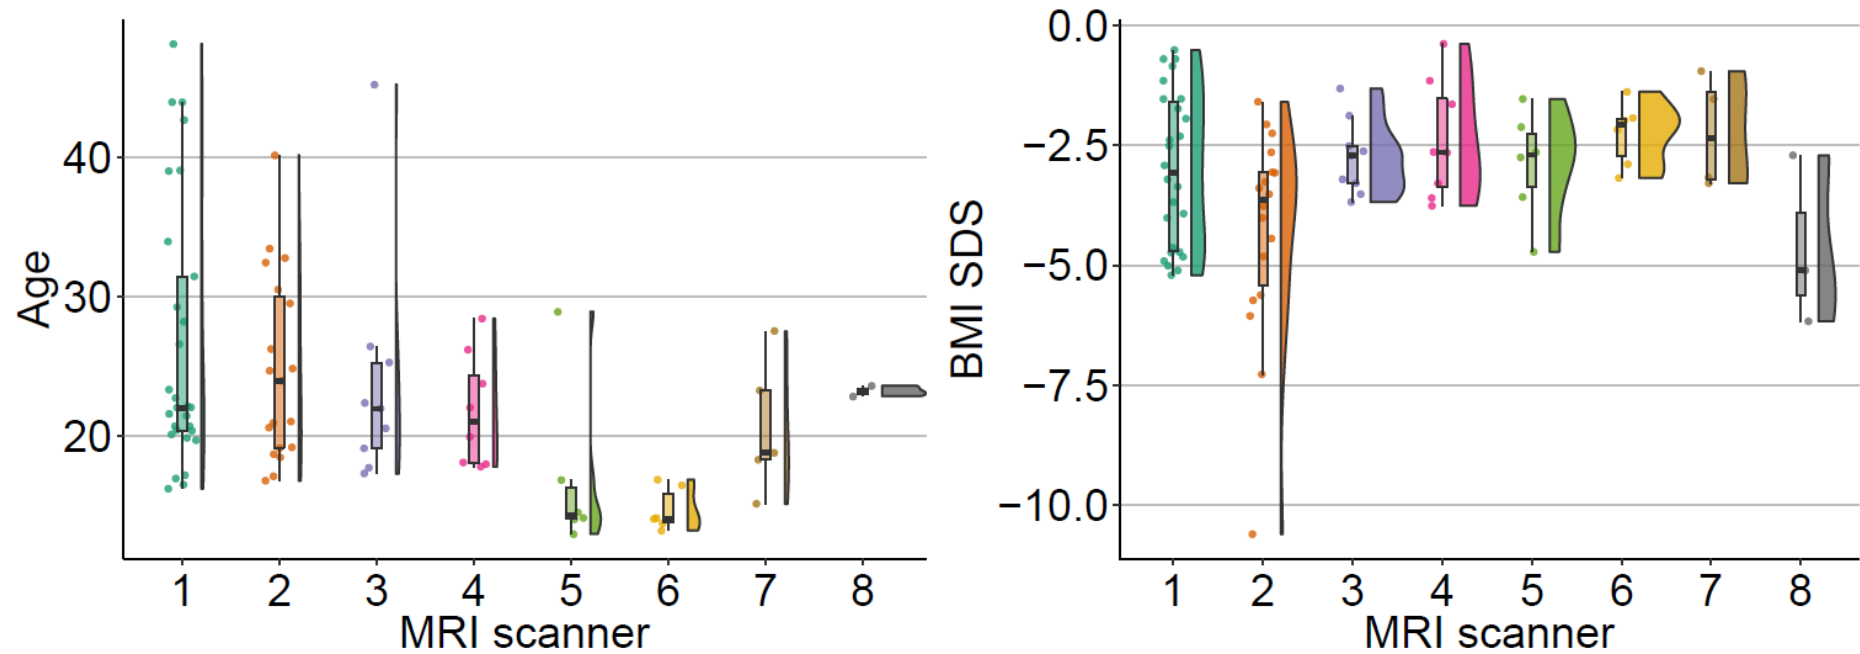


Figure S1. Raincloud plots showing distributions of age and BMI SDS across MRI scanners. MRI scanners are numbered according to Table S1-2. BMI SDS, Body mass index (kg/m^2) standard deviation score; MRI, Magnetic resonance imaging.

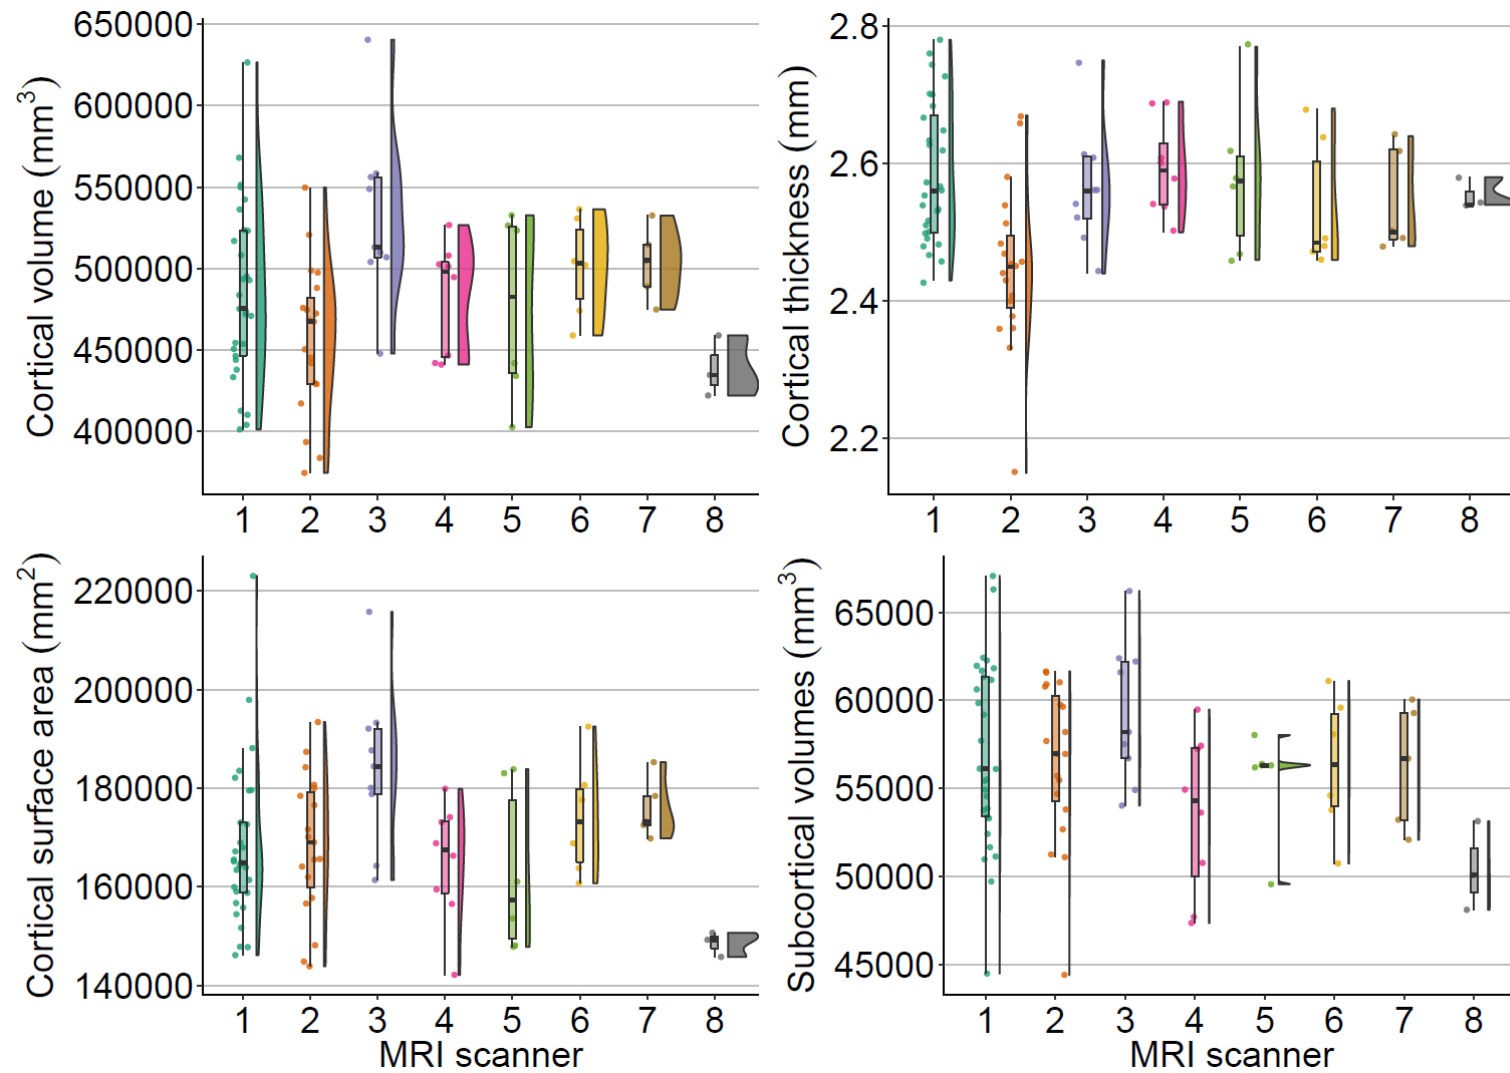


Figure S2. Raincloud plots showing distributions of brain morphology estimates across MRI-scanners. MRI scanners are numbered according to Table S1-2. Mm, Millimeters; MRI, Magnetic resonance imaging.

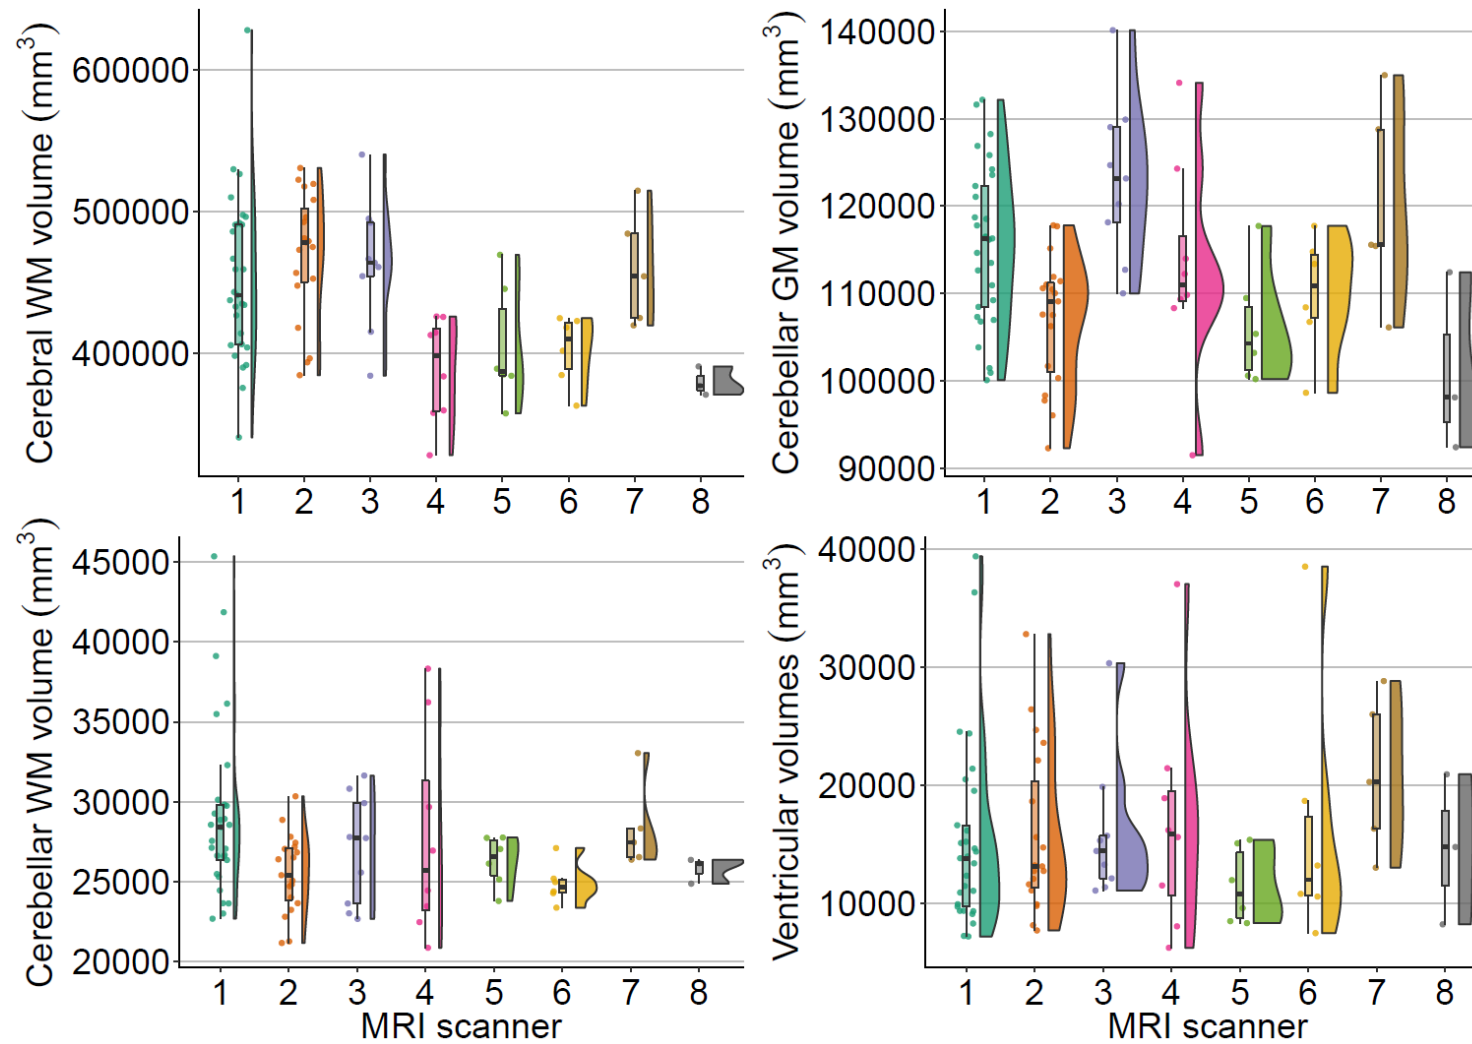


Figure S3. Raincloud plots showing distributions of brain morphology estimates across MRI-scanners. MRI scanners are numbered according to Table S1-2. GM, Gray matter; Mm, Millimeters; MRI, Magnetic resonance imaging; WM, White matter.

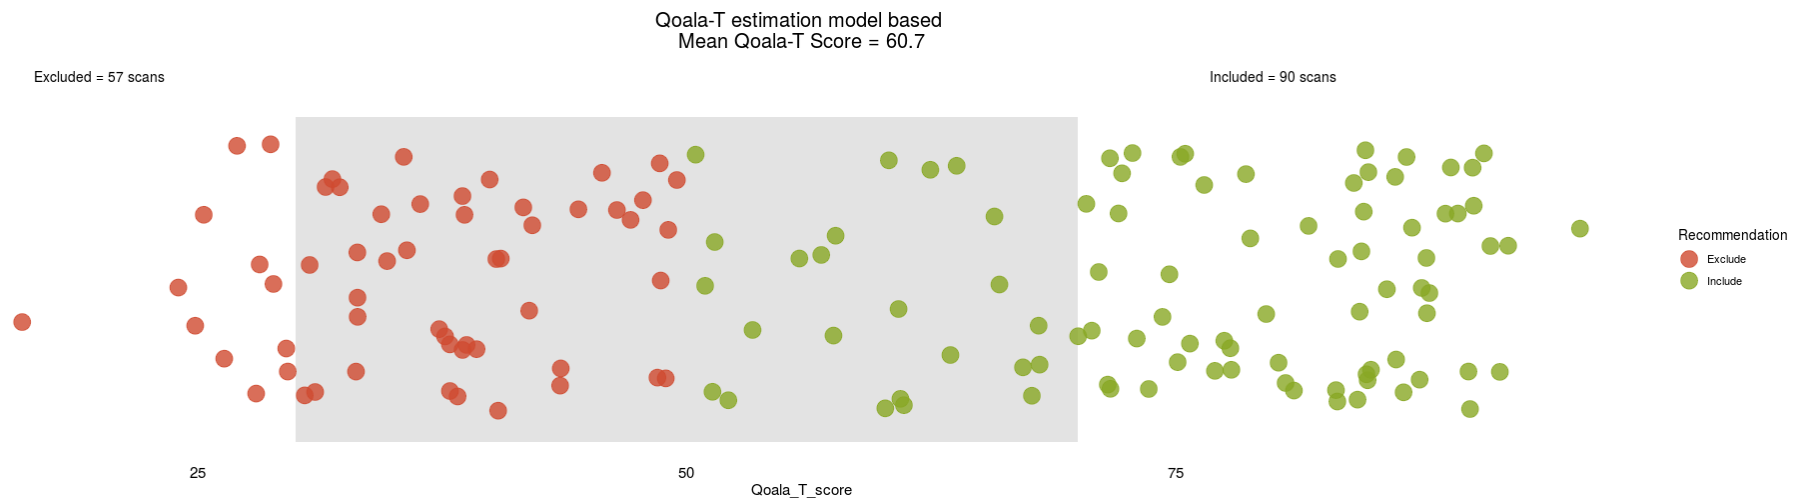


Figure S4. Results from Qoala-T quality control. Out of 212 eligible scans, 147 completed processing in FreeSurfer and were subjected to both manual and automatic quality control. The automated quality control was performed with Qoala-T, which yields recommendations for inclusion or exclusion.

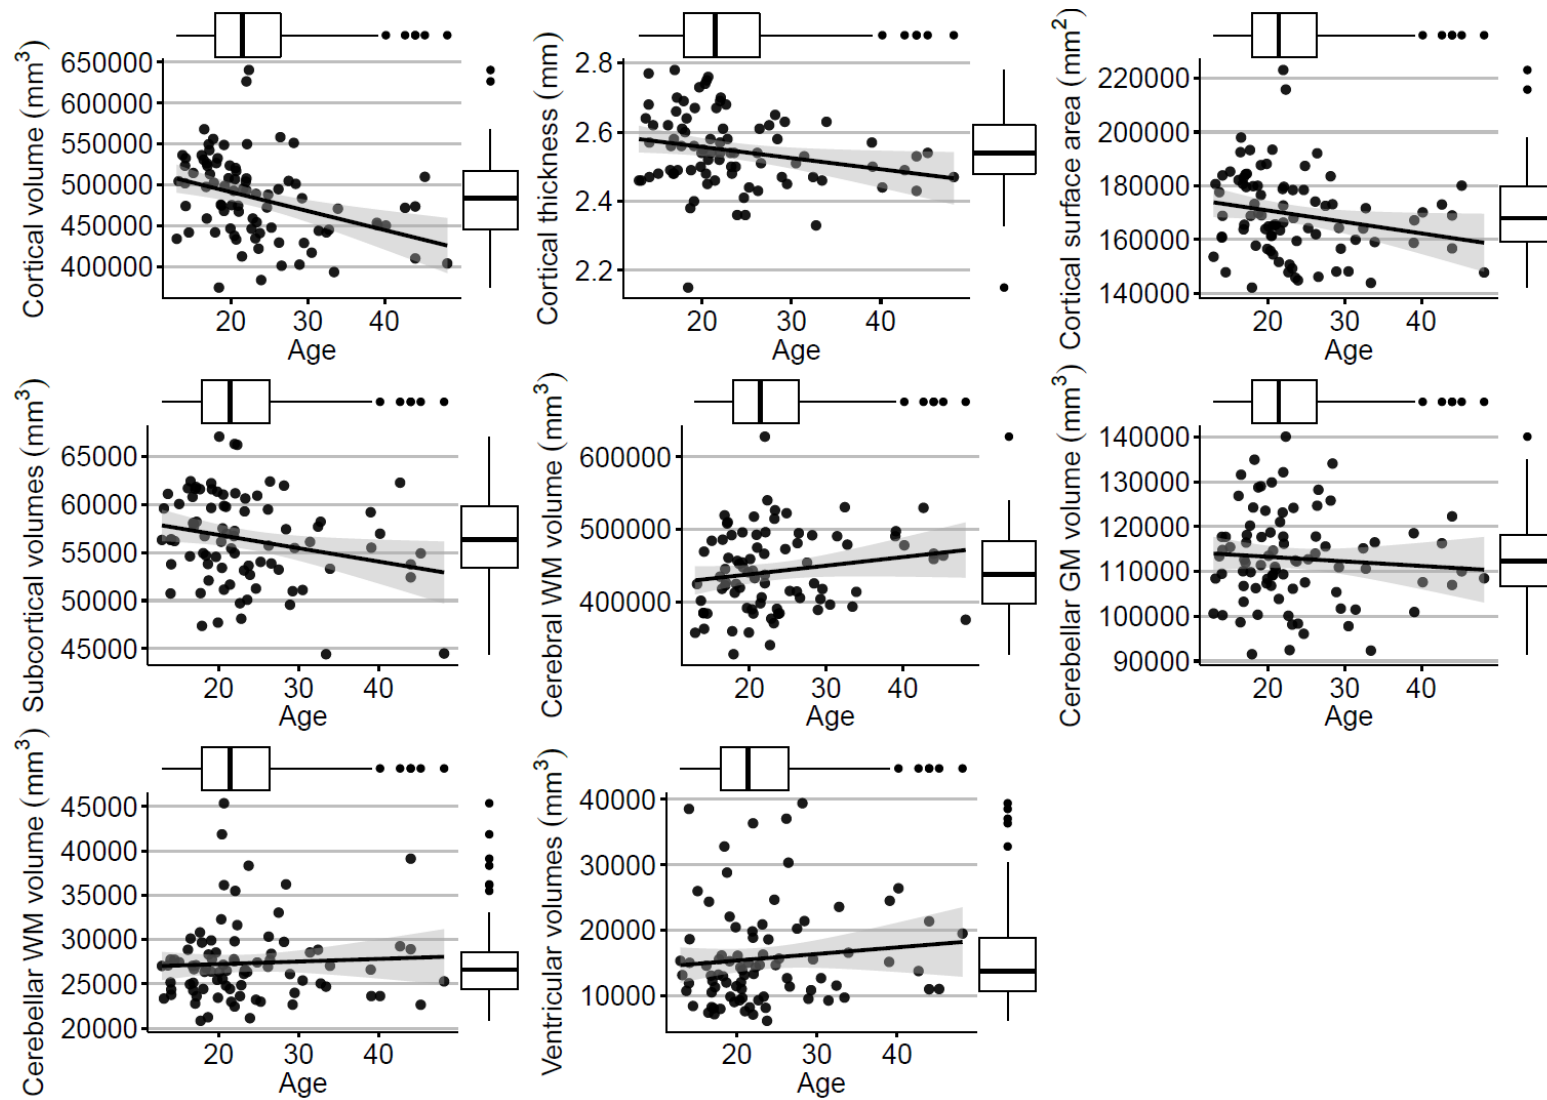


Figure S5. Scatterplots showing associations between age and brain morphology. GM, Gray matter; Mm, Millimeters; WM, White matter.

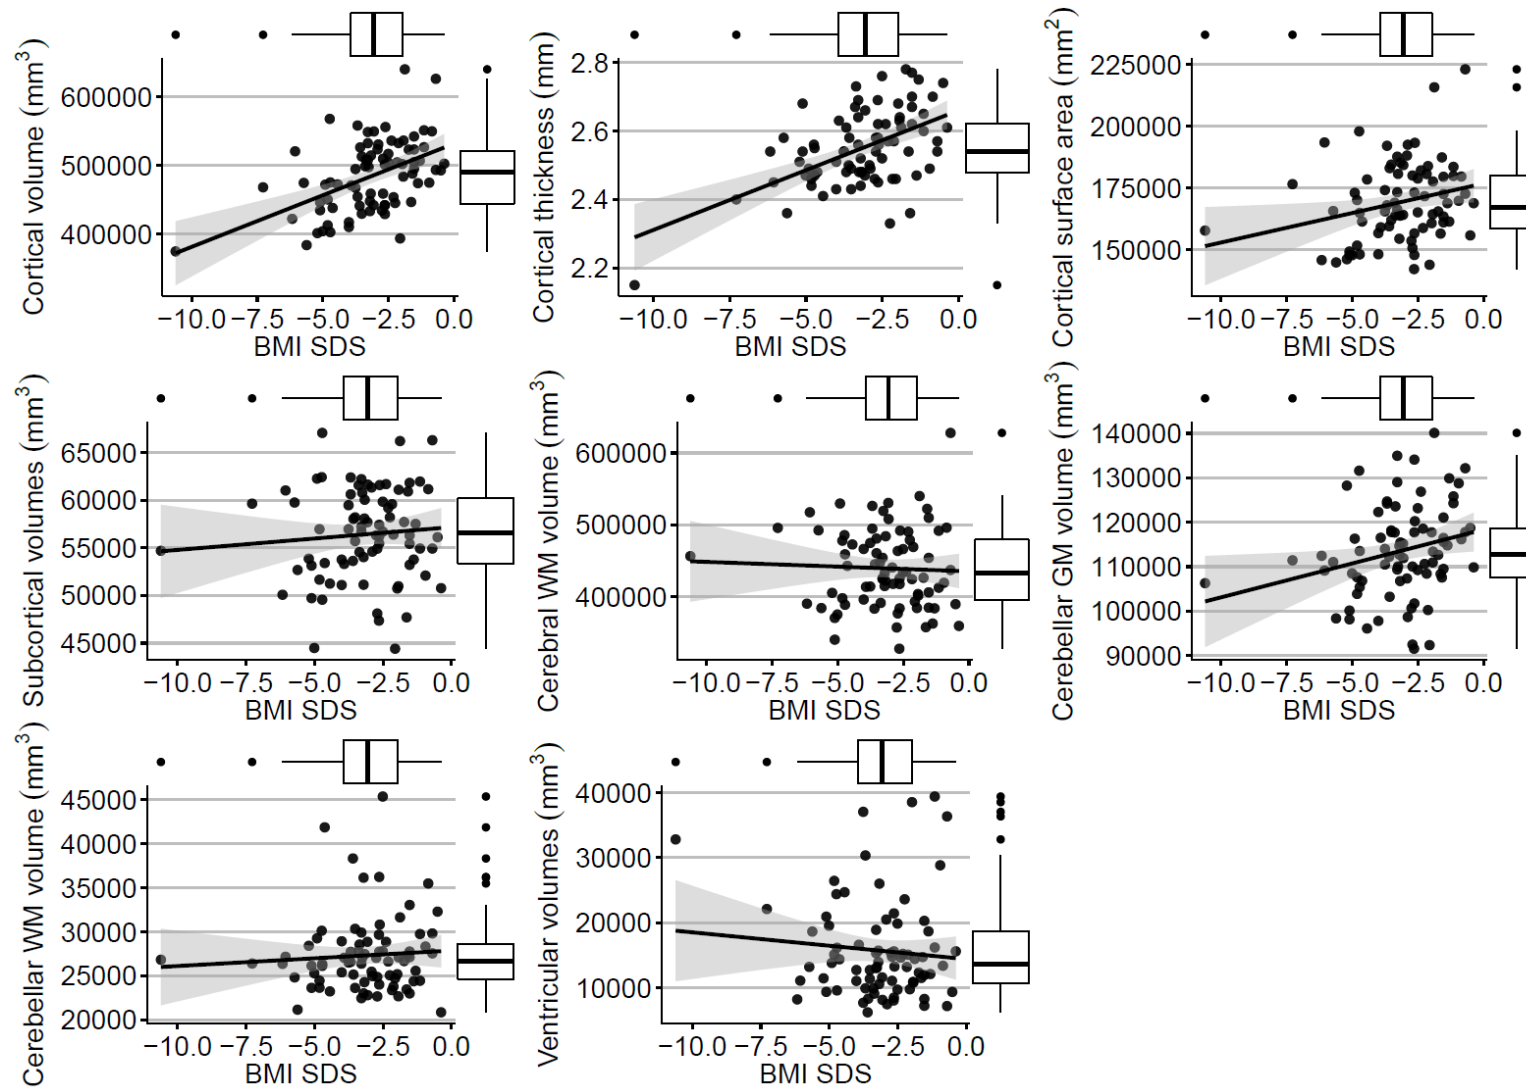


Figure S6. Scatterplots showing associations between BMI SDS and brain morphology. BMI SDS, Body mass index (kg/m^2) standard deviation score; GM, Gray matter; Mm, Millimeters; WM, White matter.

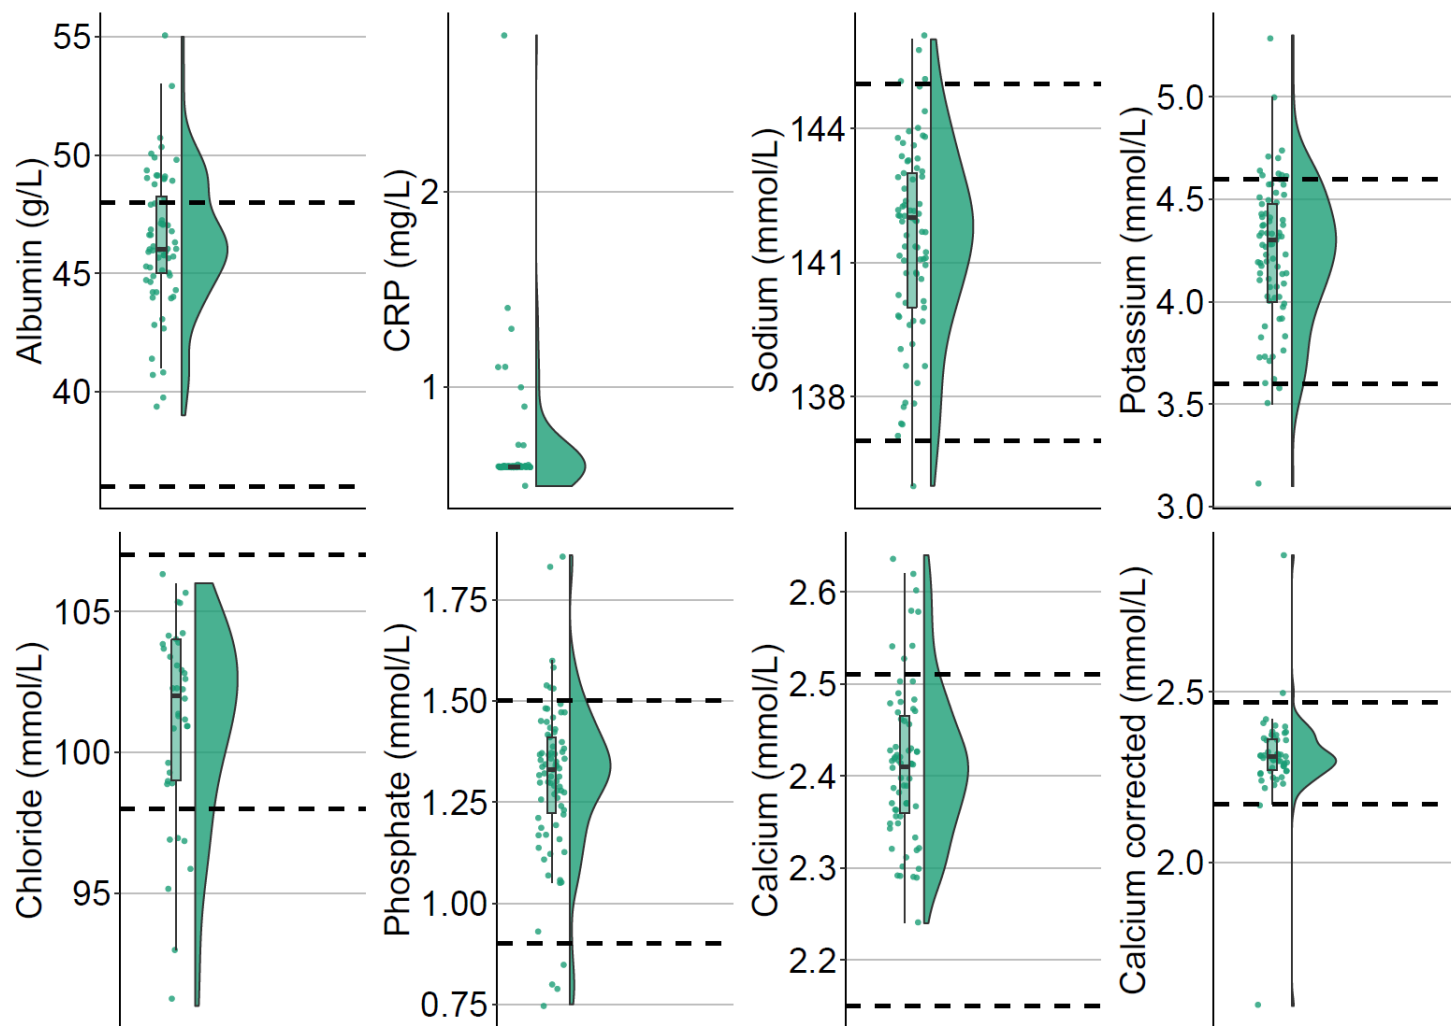


Figure S7. Raincloud plots showing distributions of biochemical parameters. Reference intervals are indicated by dashed lines (with the exception of CRP, where all patients scored within normal range). Calcium corrected, Calcium corrected for albumin levels; CRP, C-reactive protein; g/L, Grams per liter; mg/L, Milligrams per liter; mmol/L, Millimoles per liter.

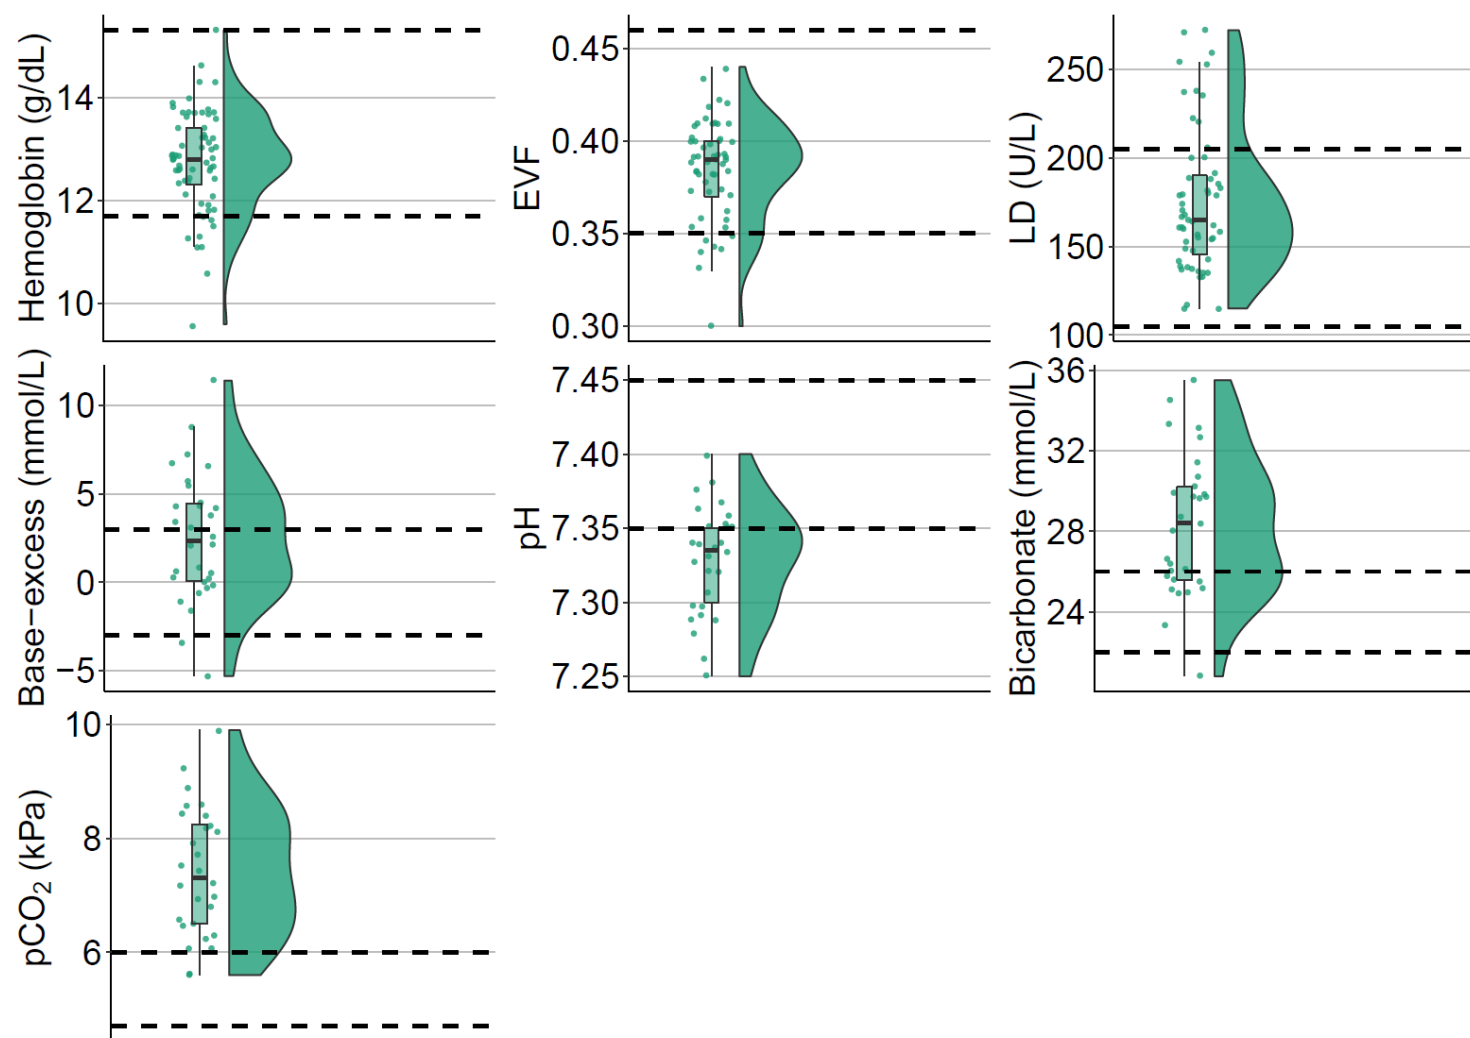


Figure S8. Raincloud plots showing distributions of biochemical parameters. Reference intervals are indicated by dashed lines. EVF, Erythrocyte volume fraction; g/dL, Grams per deciliter; kPa, Kilopascal; LD, Lactate dehydrogenase; mmol/L, Millimoles per liter; pCO₂, Partial pressure of carbon dioxide; U/L, Units per liter.